

Fig. 1 (Prior Art)

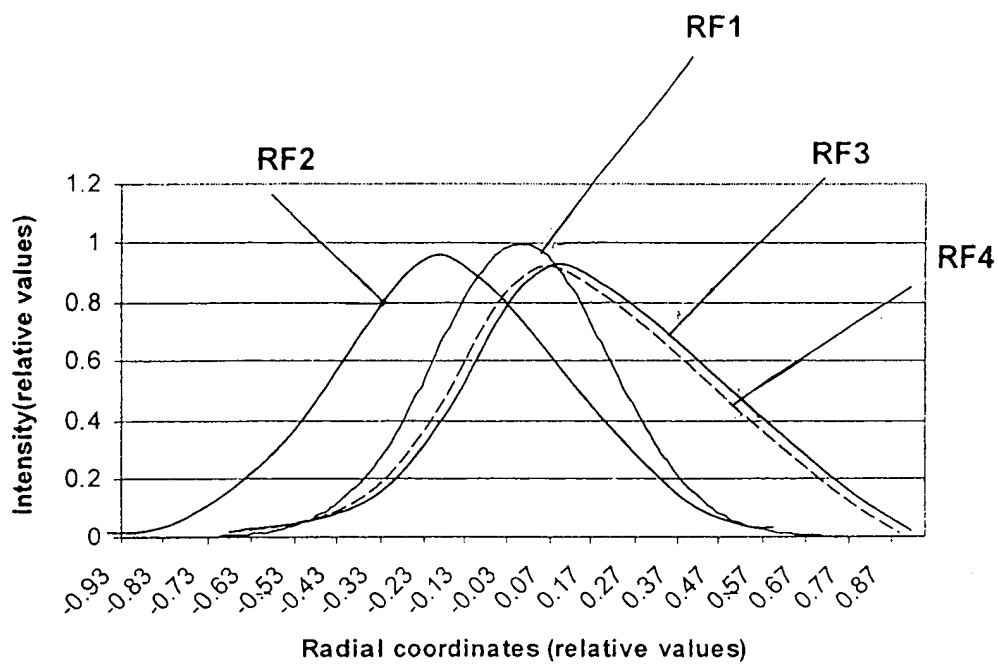


Fig. 2A



Signal values for prior art phase contrast system

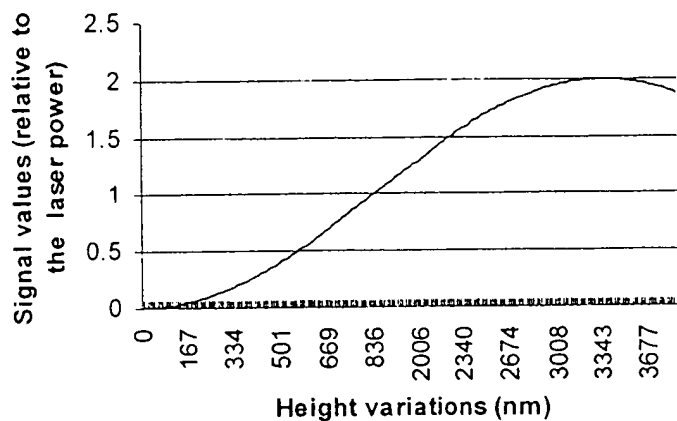


Fig. 2B

Signals for prior art phase contrast system



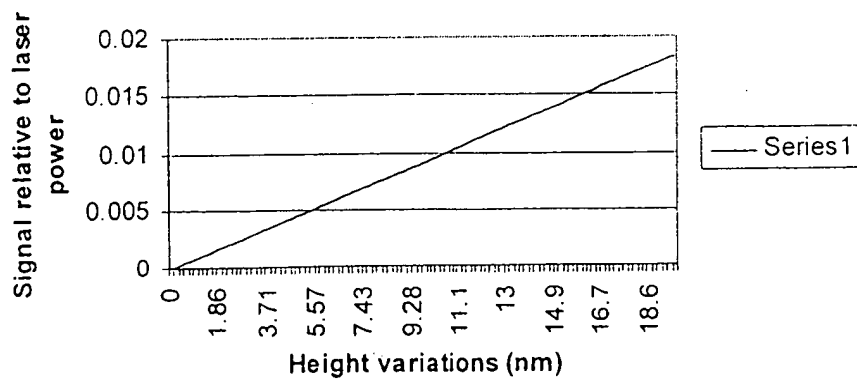


Fig. 2C



**Fig. 3**

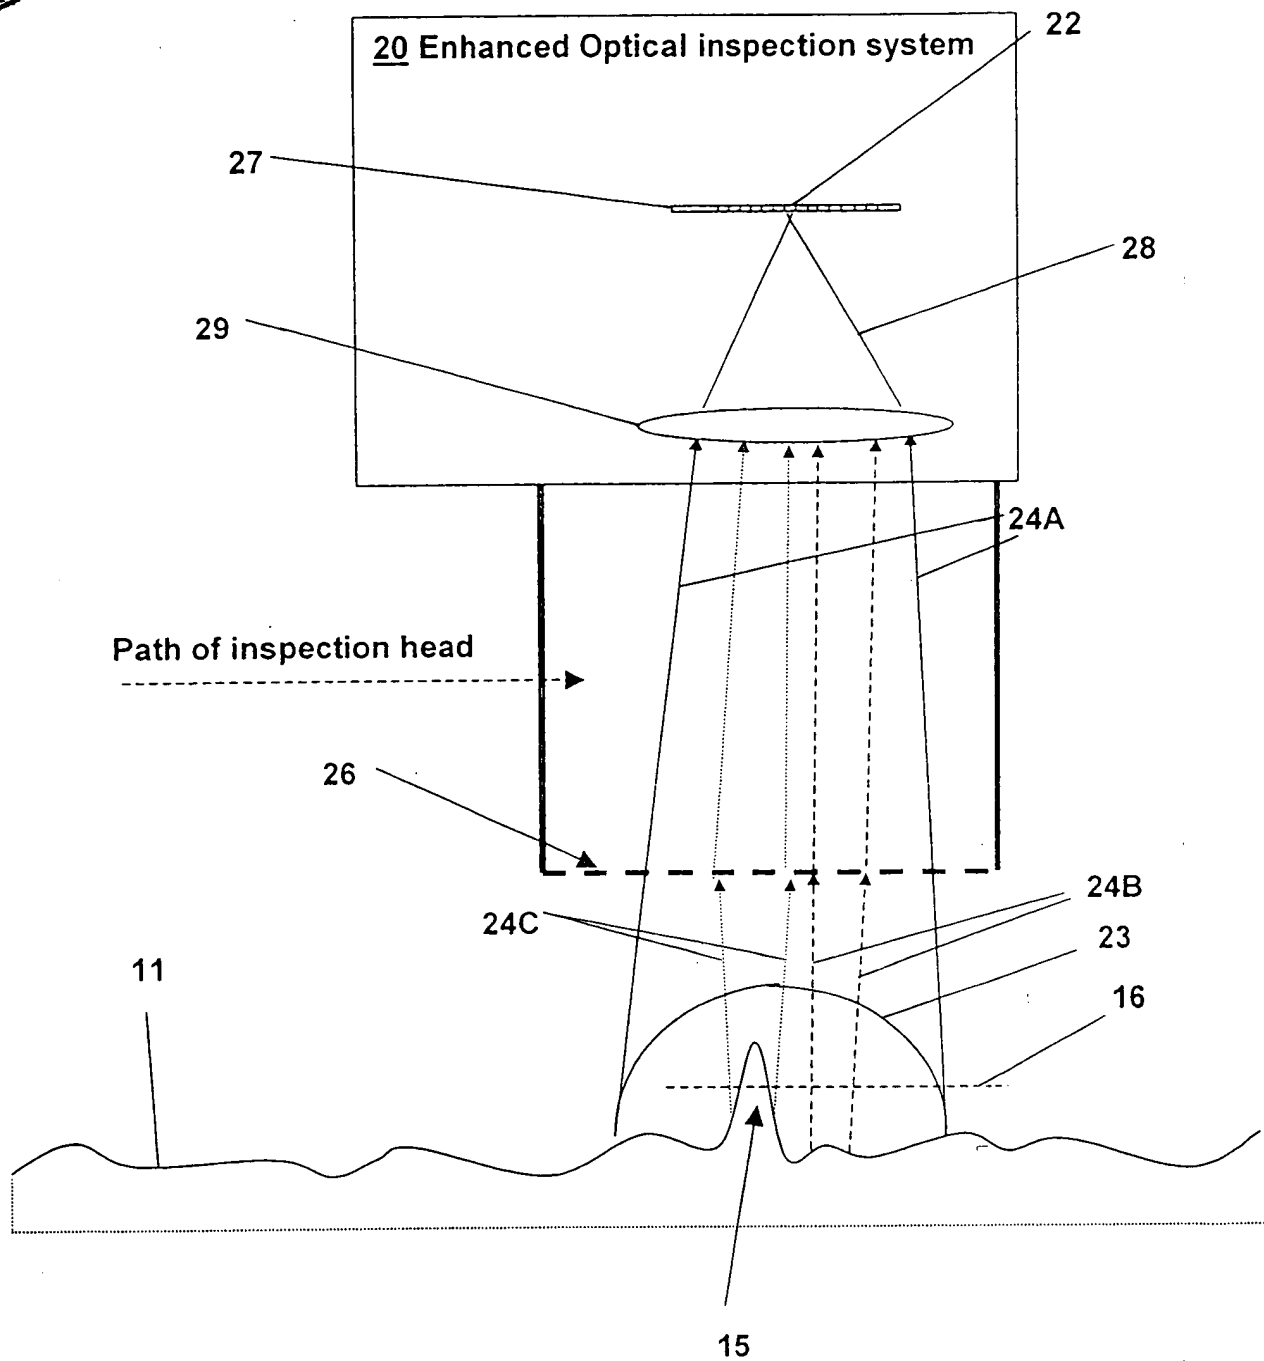

# Signal values for enhanced phase contrast system

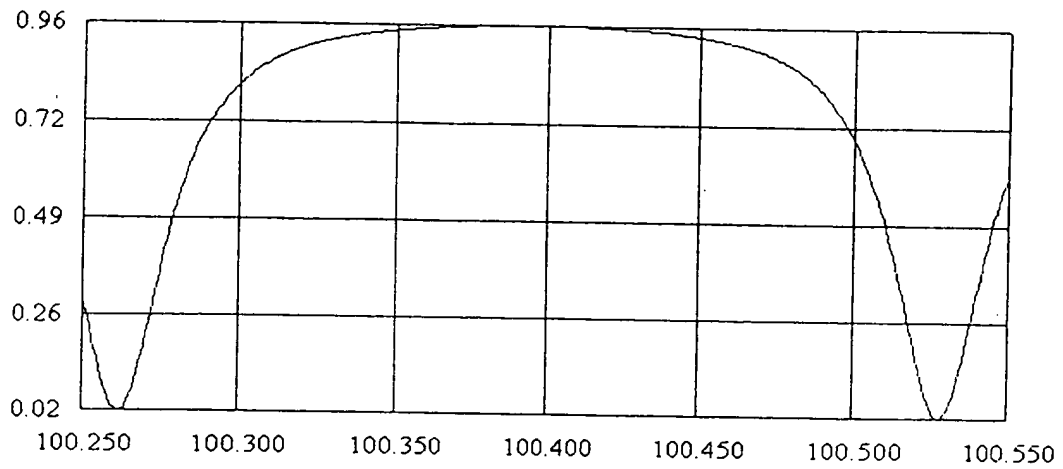


Fig. 4A

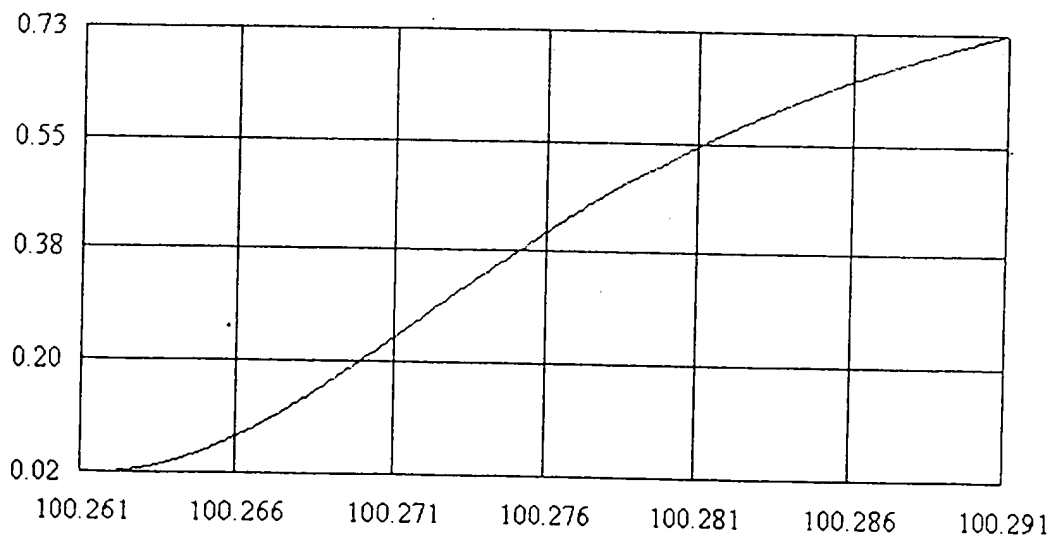


Fig. 4B

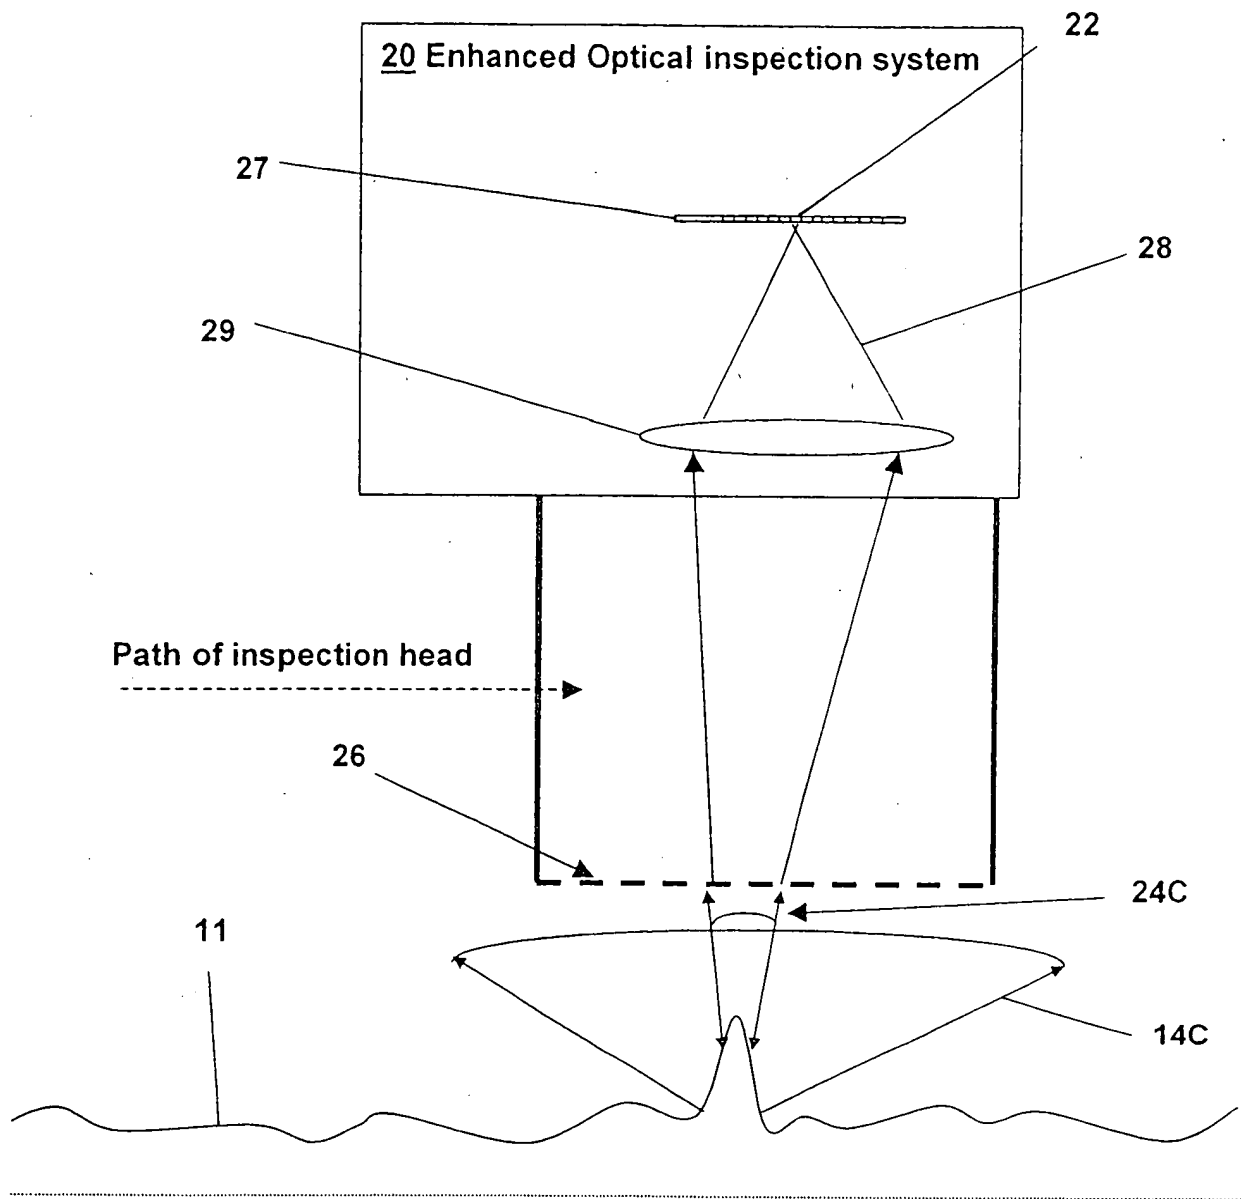


Fig. 5

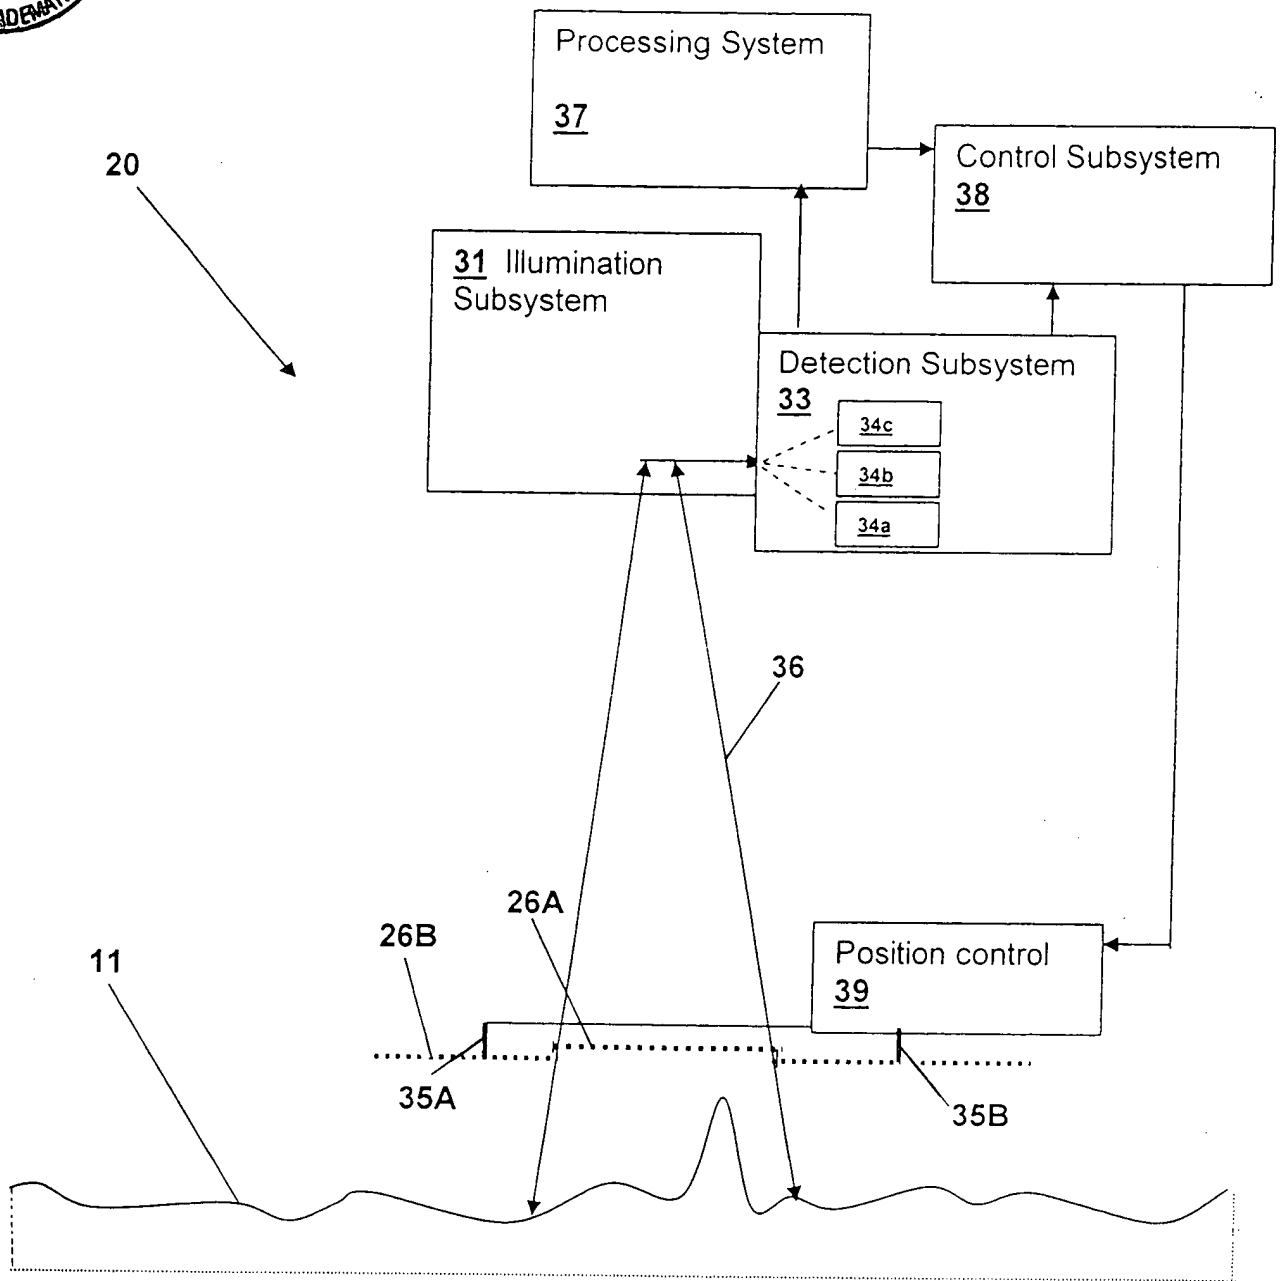


Fig. 6